



CERCON[®] Chairside Guide

zirconia


Tooth Preparation Guide

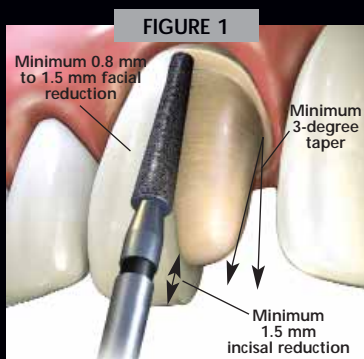


Preparation for an anterior crown is performed with a coarse diamond bur; facial reduction of 0.8 mm to 1.5 mm must be achieved.

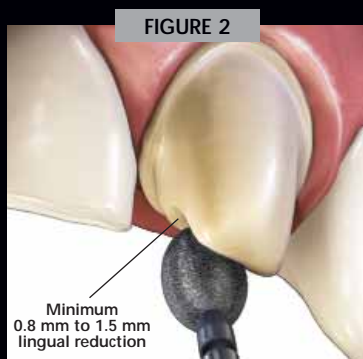

For the anterior all-ceramic crown, lingual reduction of 0.8 mm to 1.5 mm must be performed with a football-shaped bur.

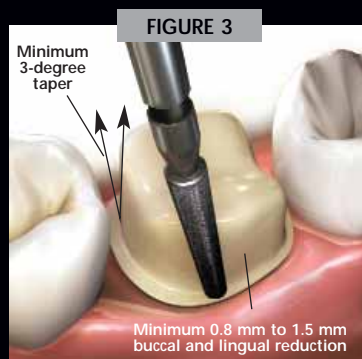

Preparation of the posterior all-ceramic crown requires at least 0.8 mm to 1.5 mm of reduction on the buccal and lingual aspects.

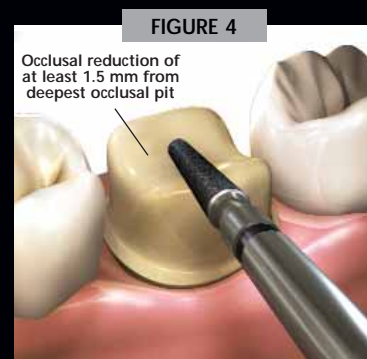


Posterior CERCON[®] Zirconia crowns require reduction of at least 1.5 mm from the deepest occlusal pit.



For a multiunit anterior CERCON® Zirconia bridge, at least 0.8 mm to 1.5 mm of reduction should be performed facially and lingually.




The multiunit anterior bridge should also have at least 1.5 mm of occlusal and incisal reduction, and it should have rounded internal line angles.

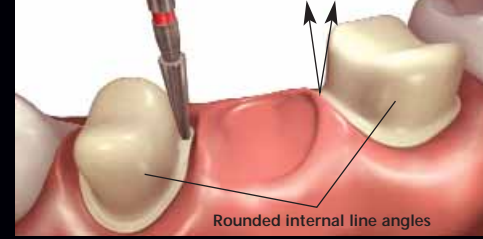


Multiunit CERCON® Zirconia bridges in the anterior and posterior require a taper of at least 3 degrees.

FIGURE 8

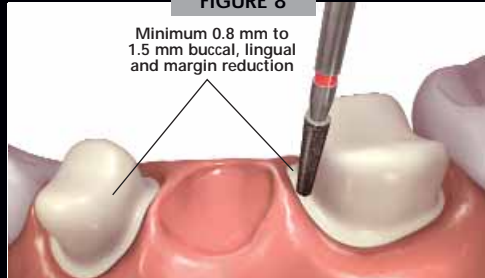


Posterior bridgework for CERCON® Zirconia also require at least 0.8 mm to 1.5 mm of buccal and lingual reduction.

FIGURE 9

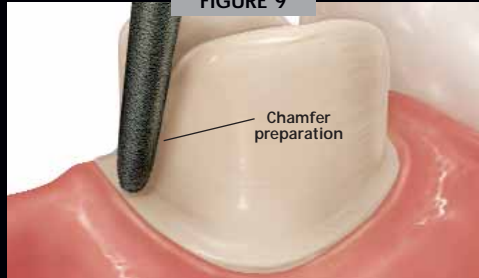

The clinician can utilize a chamfer margin design when preparing abutment teeth for the all-ceramic bridge.

FIGURE 10

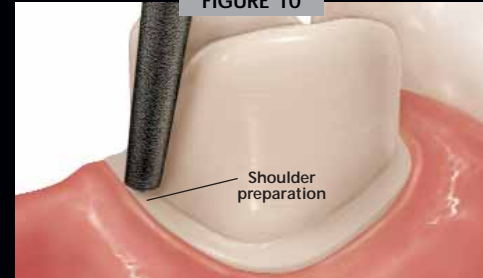

A shoulder margin design can also be used to prepare abutment teeth for the all-ceramic bridge.

DENTSPLY
CERAMCO

DENTSPLY International Inc.
570 West College Ave.
York, PA, USA 17405-0872
Tel: 800-243-1942
www.ceramco.com or
www.dentsply.com

CE|REP
DeguDent GmbH
Rodenbacher Chaussee 4
63457 Hanau-Wolfgang
Germany
Tel: +49/6181/59-50

Distributed by:
DENTSPLY Canada
161 Vinyl Court
Woodbridge, Ontario
L4L 4A3
905-968-5374

Rx only **CE**
008

REF 090781 Rev. 05/0